

Clarity Controls

Sartorius Balance

BALANCE

ENG

Code/Rev.: M056/30A
Date: 24.5.2010

Phone: +420 251 013 400
Fax: +420 251 013 401
clarity@dataapex.com
www.dataapex.com

DataApex Ltd.
Podohradská 1
155 00 Prague 5
The Czech Republic

Clarity[®], DataApex[®] and [®] are trademarks of DataApex Ltd. Microsoft[®] and Windows[™] are trademarks of Microsoft Corporation.
DataApex reserves the right to make changes to manuals without prior notice. Updated manuals can be downloaded from www.dataapex.com.

Author: DM

Contents

1 Sartorius Balance Control Module	1
2 Requirements	2
3 Installation Procedure	3
3.1 Sartorius balance communication.....	3
3.2 Clarity Configuration.....	4
4 Using the control module	6
4.1 Standard operation procedure.....	6
4.2 Get Weight.....	7
4.3 Sartorius Setup.....	8
5 Troubleshooting	9

To facilitate the orientation in the **Sartorius Balance** manual and **Clarity** chromatography station, different fonts are used throughout the manual. Meanings of these fonts are:

Instrument (blue text) marks the name of the window, to which the text refers.

Open File (italics) describes the commands and names of fields in **Clarity**, parameters that can be entered into them or a window or dialog name (when you already are in the topic describing the window).

WORK1 (capitals) indicates the name of the file and/or directory.

ACTIVE (capital italics) marks the state of the station or its part.

The bold text is sometimes also used for important parts of the text and the name of the **Clarity** station. Moreover, there are text sections written in format other than normal text. These sections are formatted as follows:

Note: Notifies the reader of possibly interesting information.

Caution: Warns the user of possibly dangerous or very important information.

█ Marks the problem statement or trouble question.

Description: Presents any closer information on the problem, describes its causes etc.

Solution: Marks the response to the question, presents a procedure how to remove it.

1 Sartorius Balance Control Module

This manual describes the setting of the **Sartorius M2P, CP, GC and GP** series balance. The control module enables direct control of the instrument over serial line.



Fig 1: Sartorius M2P balance

Direct control means that the balance can be completely controlled from the **Clarity** environment. The weight of samples can be obtained from **Clarity** and automatically transferred into the sequence table.

2 Requirements

- **Clarity** Installation CD ROM with EA Extension (p/n A30).
- Free serial COM port in the PC.

Note: Modern computers usually have only 1 (if any) serial (COM) port installed. To use more devices requiring the RS232 port, the **MultiCOM** adapter (p/n MC01) is available.

- Serial cross DB9F-DB25M cable (p/n SK03).

Note: Cables are not part of **Clarity** Control Module. It is strongly recommended to order required cables together with the Control Module.

3 Installation Procedure

3.1 Sartorius balance communication

The **Sartorius** balance are controlled by serial (RS232) communication. They use standard serial cross DB9F-DB25M cable (p/n SK03). The communication parameters on the balance and in **Clarity** are variable,

Clarity uses these values as default:

Baud rate 1200, parity N, bits 8, stop bit 1.

Furthermore, it is necessary to set some menu code settings on the balance, according to their type. These settings are:

- For the **M2P** balance, the menu code C212 (Output upon print command at stability) has to be set.
- For the **CP**, **GC** and **GP** balance, menu codes:

211 (Weighing)


551 (SBI(ASCII))

612 (Manual at stability)

721 (For raw data (16 characters))

has to be set. The process of setting these parameters is described in the **Sartorius Balance** hardware manual.

3.2 Clarity Configuration

- Invoke the [System Configuration](#) dialog accessible from the [Clarity](#) window using the *System - Configuration* command.
- Press the [Add](#) button  to invoke the [Available Control Modules](#) dialog.

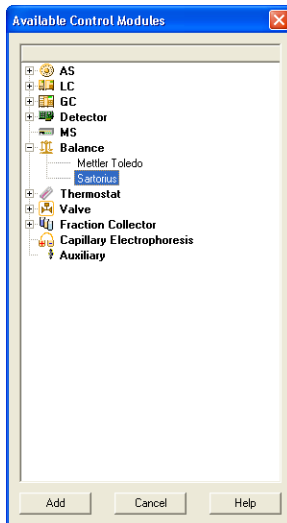


Fig 2: Available Control Modules

- Select the **Sartorius** from the **Balance** group and press the [Add](#) button.
- The [Sartorius Setup](#) dialog will appear.

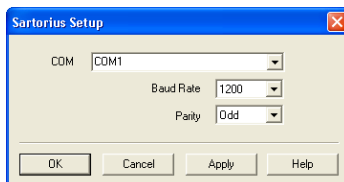









Fig 3: Sartorius Setup

- Select the correct *COM* port and set the *Baud Rate* and *Parity* so that these parameters correspond to the same parameters set in the hardware. [Sartorius Setup](#) dialog is more closely described later in the manual (for more details see also chapter [Sartorius Setup](#) on pg 8).
- The **Sartorius** item  will appear in the *Setup Control Modules* list of the [System Configuration](#) dialog.
- The instrument must be set to the **EA** mode  to be able to use balance on it.

- Drag the Balance icon  from the *Setup Control Modules* list on the left side to the desired *Instrument* tab  on the right side , or use the  button  to do so.

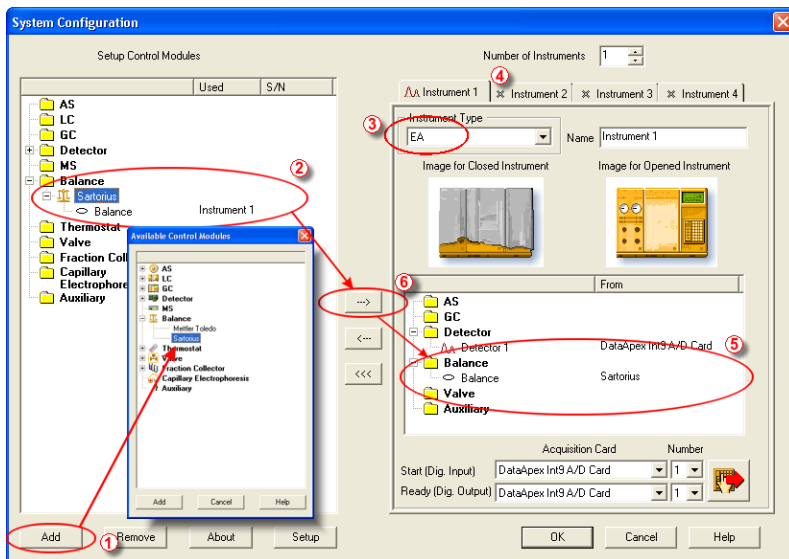



Fig 4: System Configuration

4 Using the control module

The display of the **Instrument** window changes after the **Clarity** Instrument is switched into the **EA** mode in the **System Configuration** dialog. These changes are described in detail in the EA Extension manual.

The **Sartorius Balance** control module doesn't add any windows or tabs to the EA Instrument window, but allows for the direct insertion of the sample weights into the EA-modified **Sequence Table**.

4.1 Standard operation procedure

- In the **Sequence** window, mark the *Sample Amount* field on the line where you want to transfer the value or the entire line. You can mark more fields/lines at the same time - values will be transferred sequentially after each use of the *Get Weight* button.
- Open the **Get Weight** dialog using the *Sequence - Balance...* command or the  icon ①.

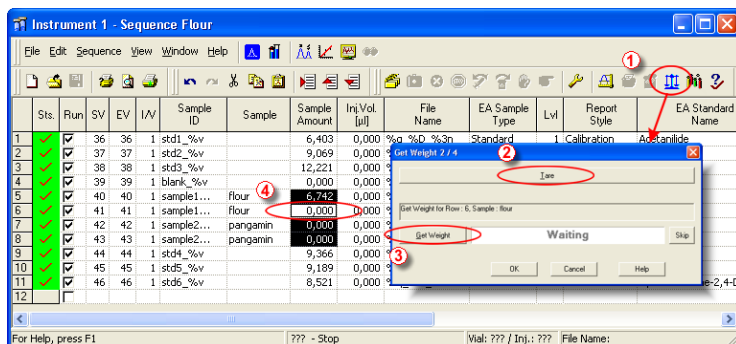


Fig 5: Standard operation procedure

- If necessary, use the *Tare* button ② to subtract the weight of an empty container.
- Place the container with sample on the balance.
- Use the *Get Weight* button ③ to transfer the weight from the analytical balance directly into the *Sample Amount* ④ field of the **Sequence Table**.

Note: Function can be used only for lines where analysis did not take place.

4.2 Get Weight

The **Get Weight** dialog is used for acquiring the weight and its automatic transfer into the *Sample Amount* fields of the **Sequence Table**. The numbers behind the "Get Weight" inscription in the name of the dialog show the number of the sample to be weighted and the total number of samples selected for weighting. The **Get Weight** dialog is opened by *Sequence - Balance...* command from the **Sequence** window.

Note: You can also open the **Get Weight** dialog using the  icon from the **Sequence** window.

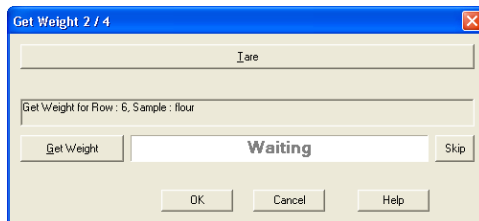


Fig 6: Get Weight

Tare

Subtracts the weight of an empty container.

Information Panel

Displays messages from the **Sequence Table** indicating current sample.

Get Weight

Transfers the weight from the analytical balance directly into the *Sample Amount* field of the **Sequence Table**.

Status Panel

Displays current status of the analytical balance. Refer to the Mettler Toledo balance documentation for description of the individual states.

Skip

Skips current sample.

4.3 Sartorius Setup

The **Sartorius Setup** dialog sets the communication settings of the control module.

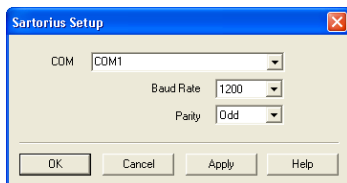


Fig 7: Sartorius Setup

COM

Sets the COM Port used for communication between the balance and the PC.

Baud Rate

Sets the speed of data on the COM Port used for communication between the balance and the PC.

Parity

Sets the parity of the data used for communication between the balance and the PC.

Note: For successful communication, all of these settings must correspond to the settings of the balance.

5 Troubleshooting

When the remedy for some problem cannot be discovered easily, the recording of communication between **Clarity** and the balance can significantly help the **DataApex** support to discover the cause of the problem.

The recording can be enabled by adding or amending the COMMDRV.INI file in the **Clarity** installation directory (C:/CLARITY by default). The file can be edited in any text editor (e.g. Notepad). Following section should be edited or added:

```
[COM1]
echo=on
textmode=on
filename=Sartorius.txt; %D or %d could be used to include a current
date (recommended in combination with the Reset=Off option
reset=off
```

Note: Instead of COM1 type the correct serial port used to communicate with the **Sartorius Balance**. This port number is displayed in the [Sartorius Setup](#) dialog.

The created *.TXT files will greatly help in diagnosis of unrecognized errors and problems in communication.